


EDX-3 Portable X-ray Spectrometer

Sample Name	insize-001	Measure Time	15s
Sample Supplier	Instrument	Voltage	45.0
Operator	QC	Current	10.0
Measure Date	2023-08-15 15:18:49	Curve	Stainless Steel
GPS	0, 0	Grade	304
Element	Content	Limit	Error
Fe (%)	71.56	0.0000	0
Cr (%)	18.25	0.0000	0
Ni (%)	8.32	0.0000	0
Mn (%)	1.34	0.0000	0
Mo (%)	0.11	0.0000	0
Cu (%)	0.30	0.0000	0
Sn (%)	0.02	0.0000	0
Zn (%)	ND	0.0000	0
Pb (%)	ND	0.0000	0
Ti (%)	0.01	0.0000	0
Co (%)	ND	0.0000	0
V (%)	0.09	0.0000	0


Spectrum

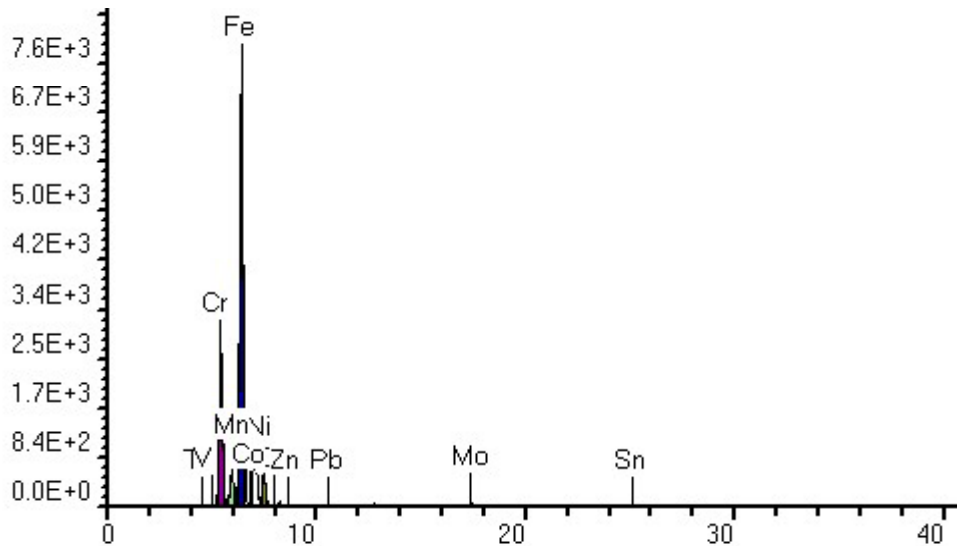

Attention: if content blow or equal limit will show ND.

EDX-3 Portable X-ray Spectrometer

Sample Name	32u	Measure Time	10s
Sample Supplier	3V Instrument	Voltage	45
Operator	QC	Current	10
Measure Date	2023/5/9 9:24	Curve	Ag-Cu
GPS	,, ,,		
Coating No.	Element	Content	Thickness
1#	Ag	-	32.0000um
2#	Cu	-	0.0000um

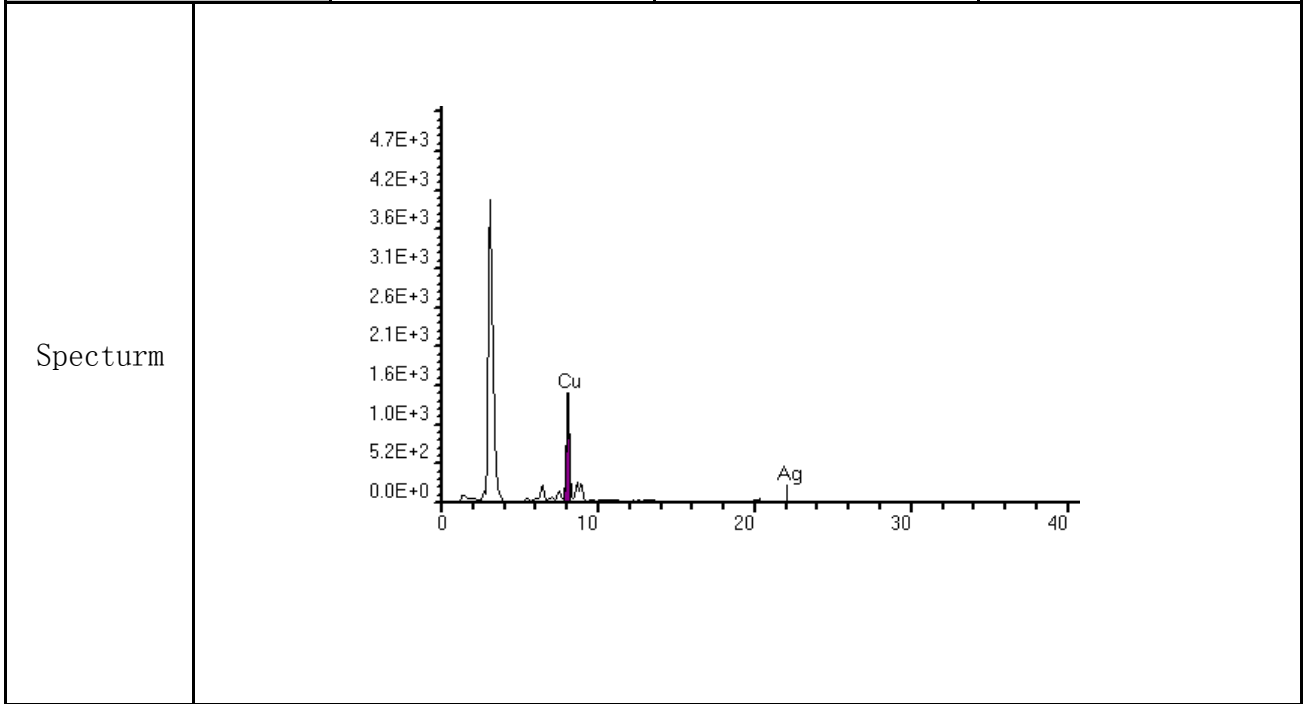

Attention: "-" indicates that the content is not calculated.